



VISIT...

LANZAROTE
Caliente.COM

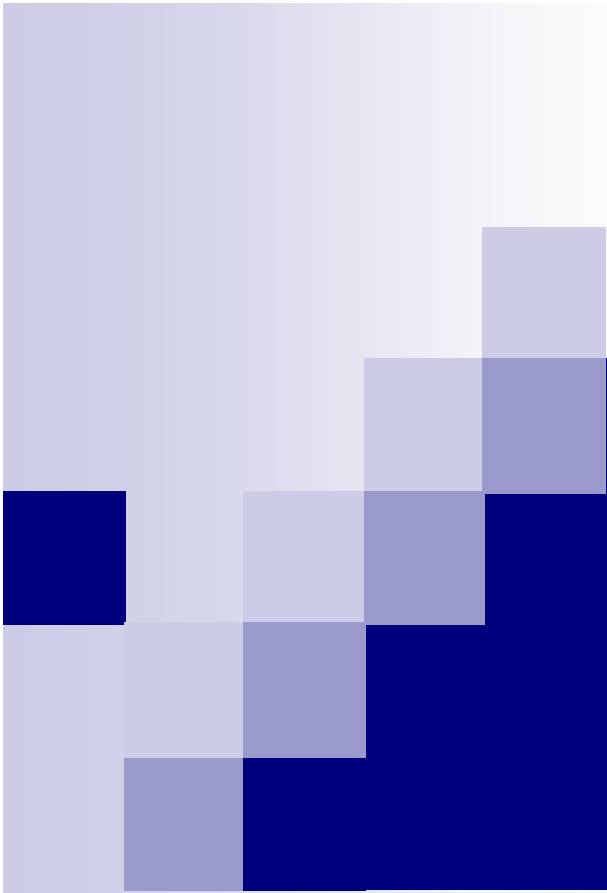


Of Monkeys and Men

Nick Annetta



Outline


- Why neuroprosthetics?
- Biological background
- 2 groups
 - University of Reading
 - University of Pittsburgh
- Conclusions




Why Neuroprosthetics?

- Amputations
 - Paralysis
 - Spinal cord injuries
 - Stroke
 - Neurological diseases
 - Amyotrophic lateral sclerosis (ALS)
 - Multiple sclerosis
 - Muscular dystrophy
- Locked-in syndrome

Biological Background

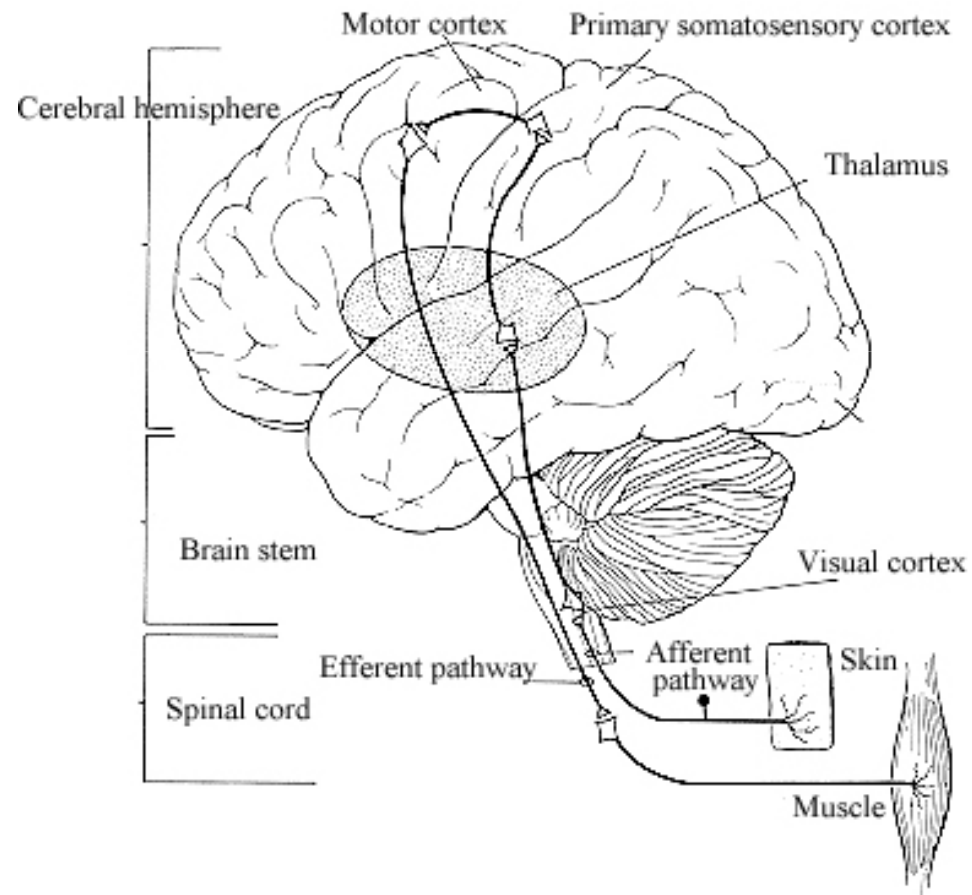




2 Groups

- University of Reading (UK)
 - Direct bi-directional prosthetic hand
 - Interface with median nerve of human left arm


- University of Pittsburgh
 - Indirect bi-directional control of prosthetic arm
 - Interface with motor cortex in monkey

Reading

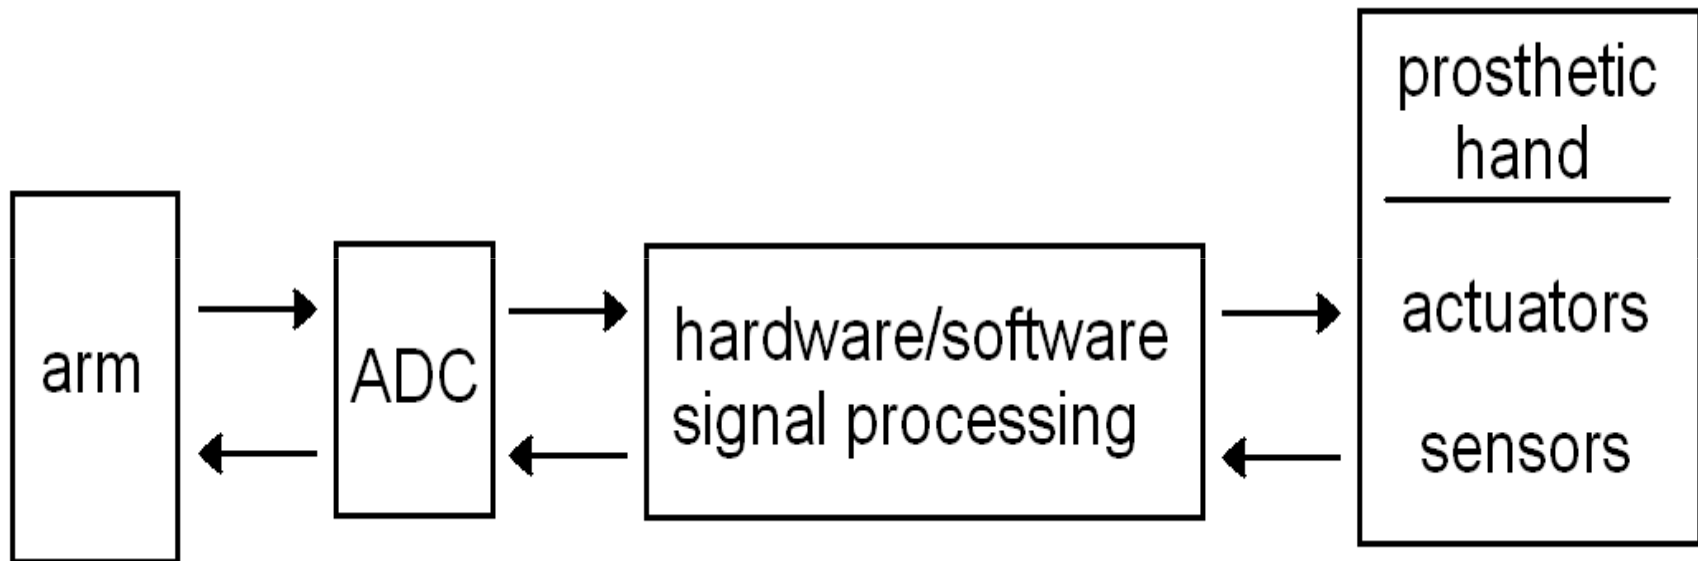

Electrode Array

- 100 electrodes
- 4x4 mm, 1.5mm length

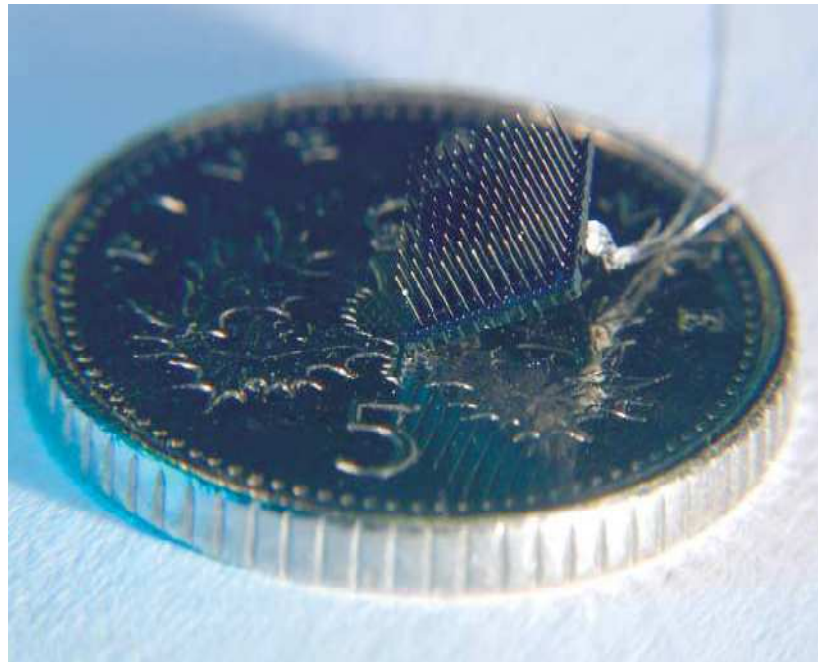

Implantation

- Median nerve



Hardware





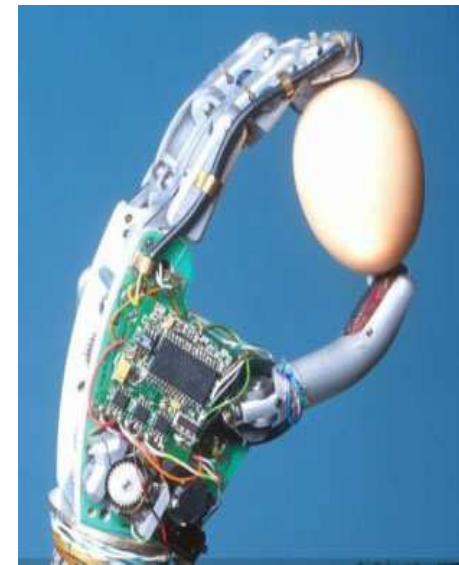


Image Source: [1,2]

Current Source

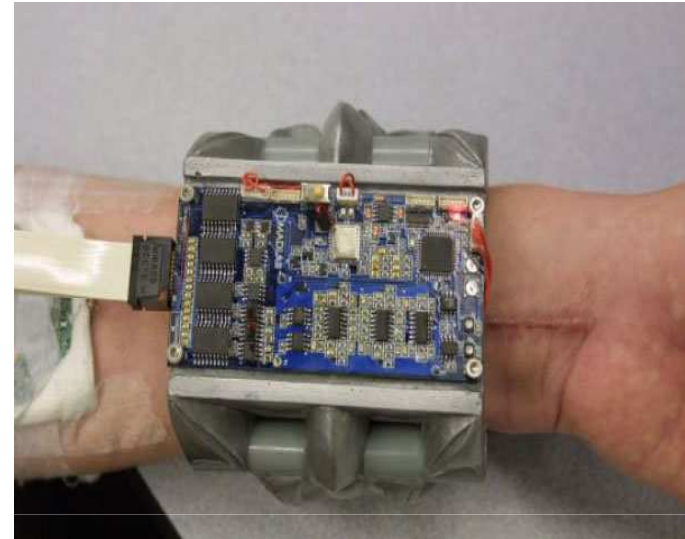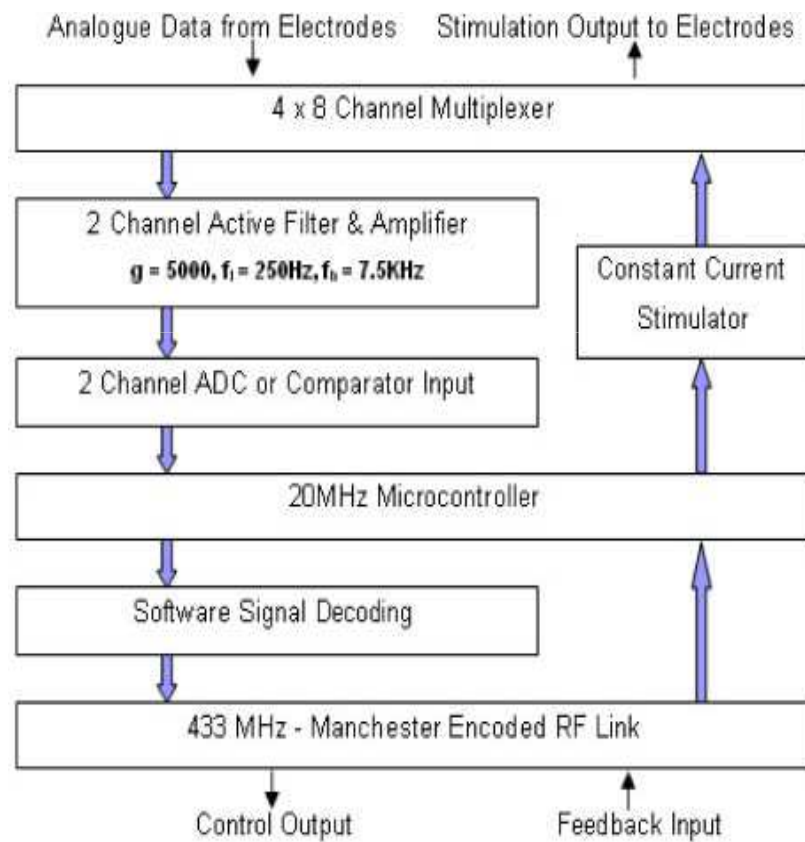
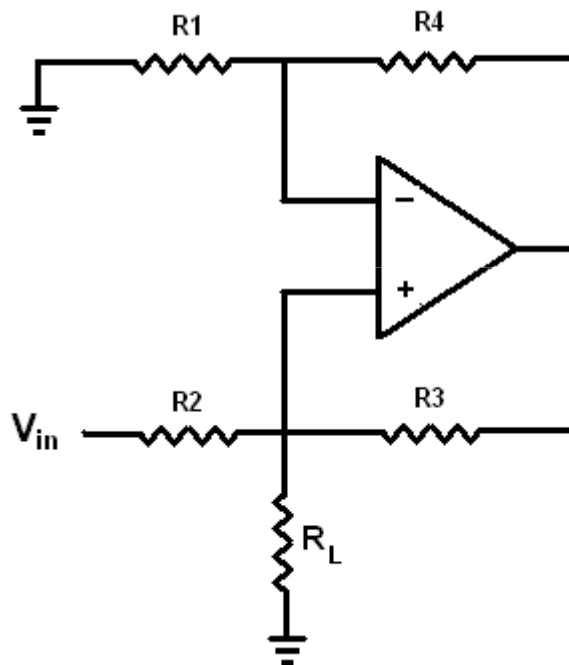


■ Howland configuration


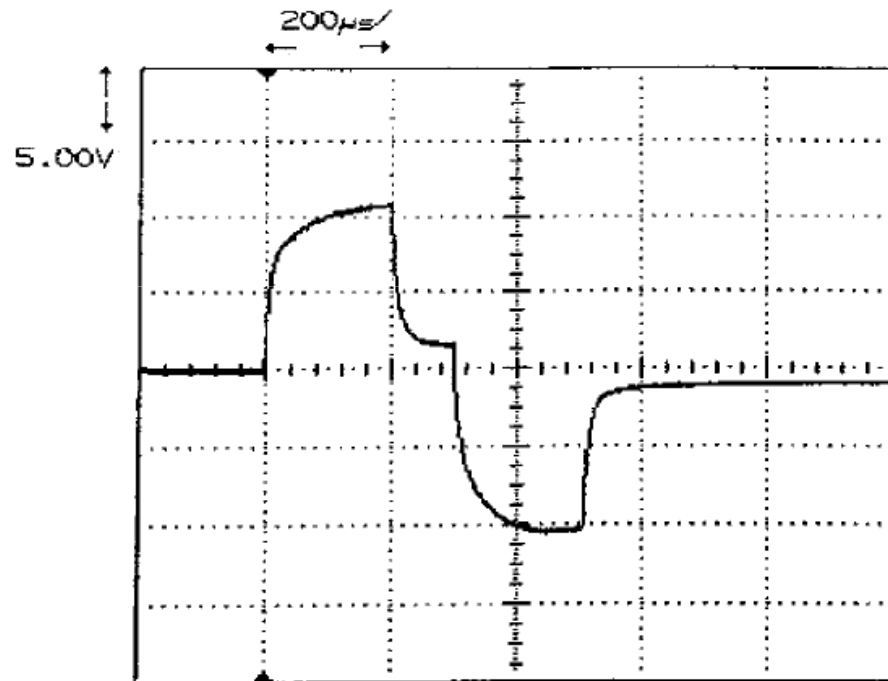


■ Single bi-phasic pulse

Results

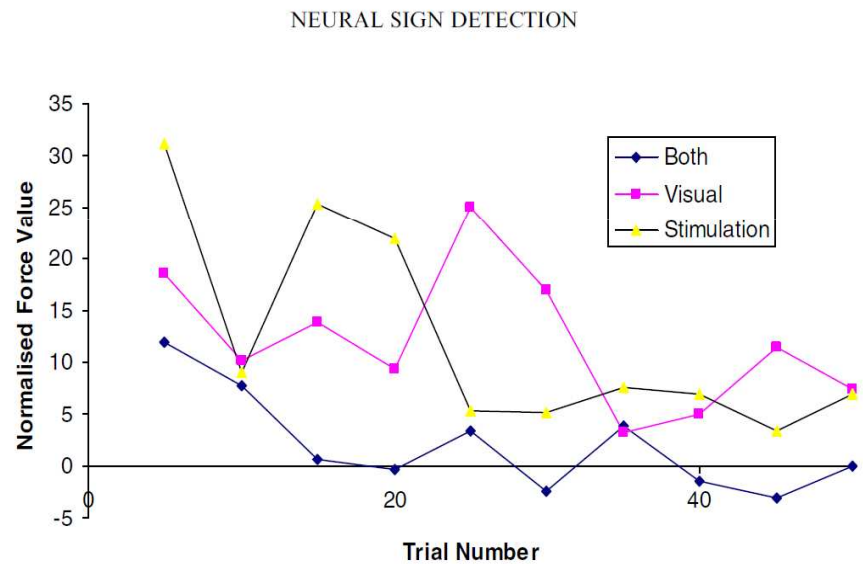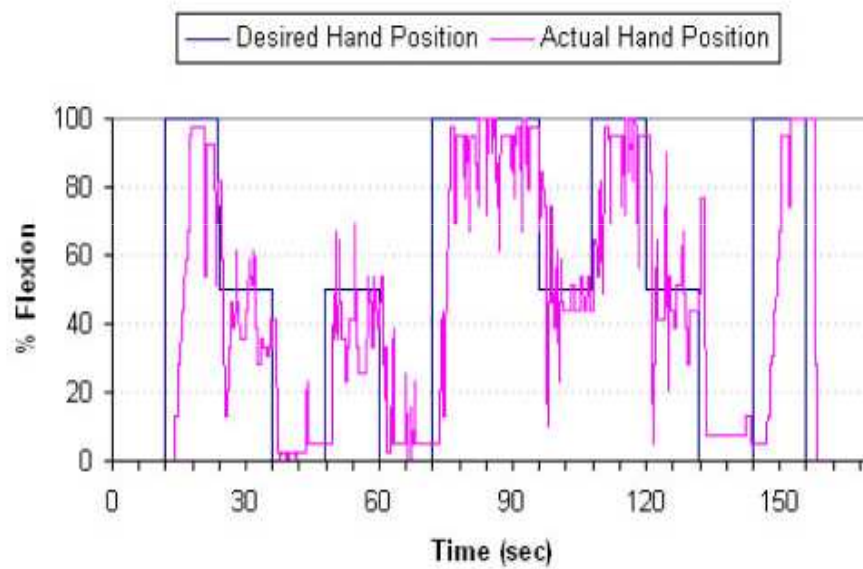


Pittsburgh

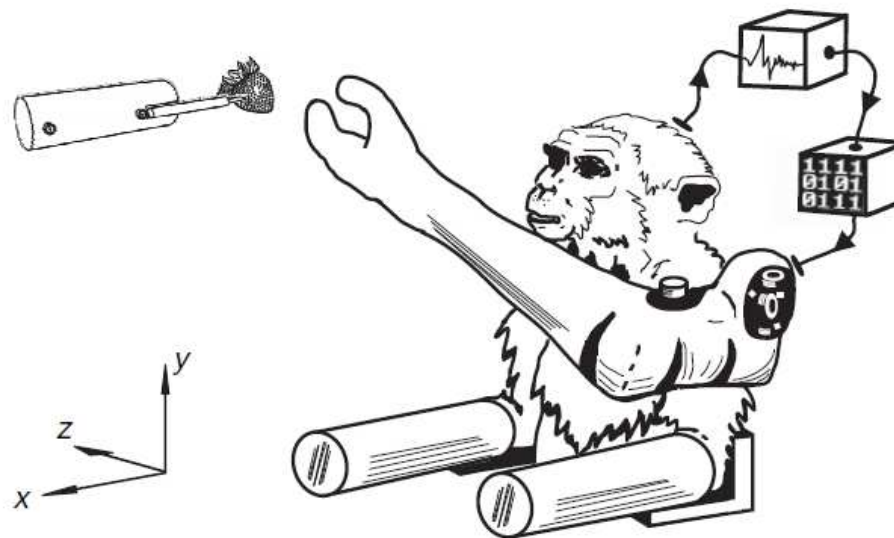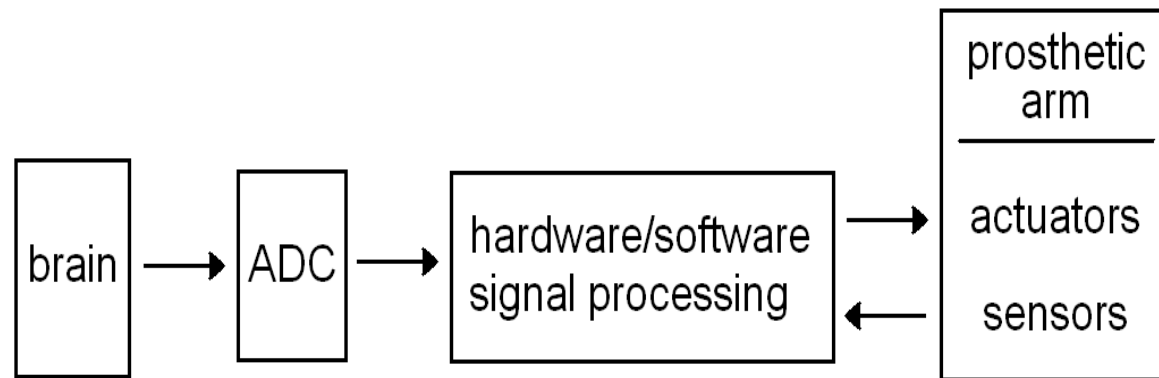


Population Vector


- Firing Rate = $a_0 + a_1X + a_2Y + a_3Z$
- Pop vector = $[a_1, a_2, a_3]$

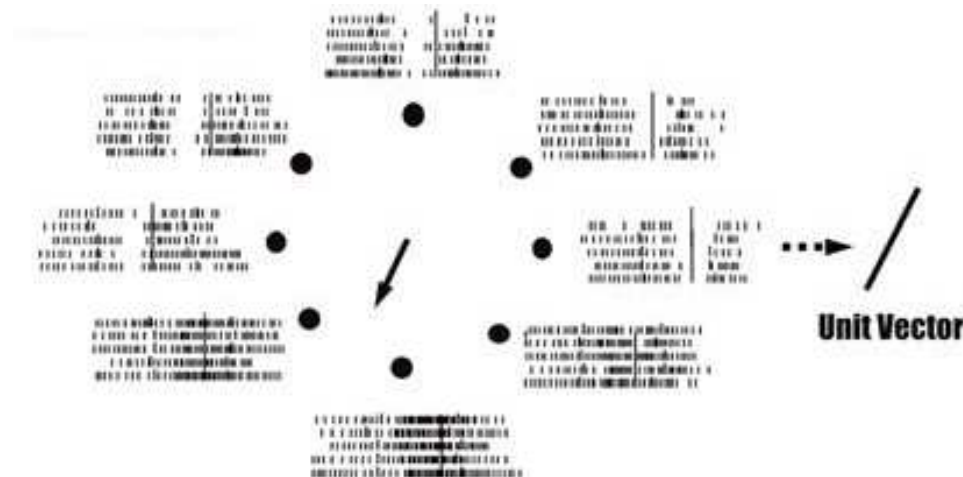

Adaptive Algorithm

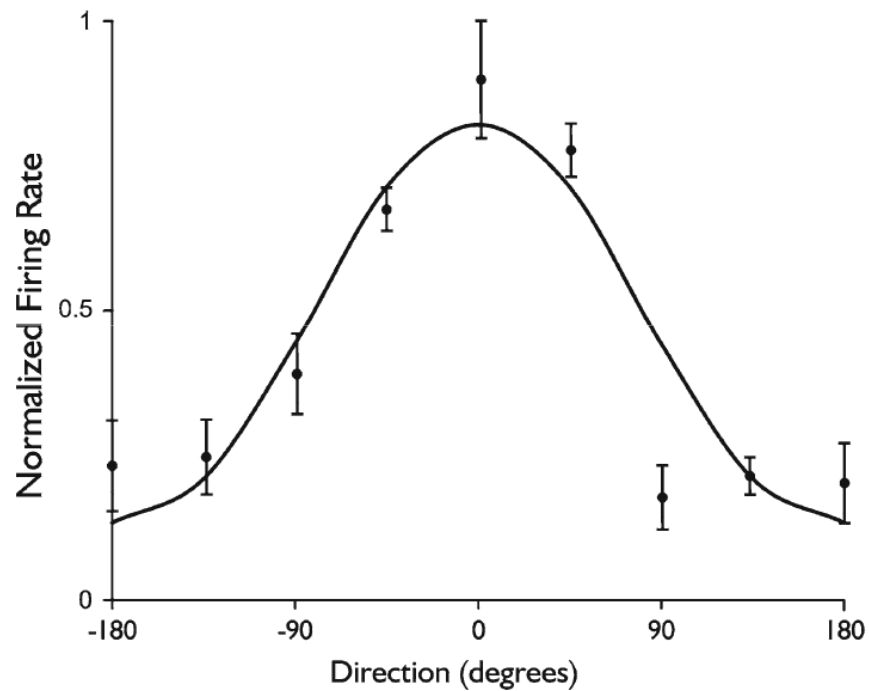


- Cosine tuning

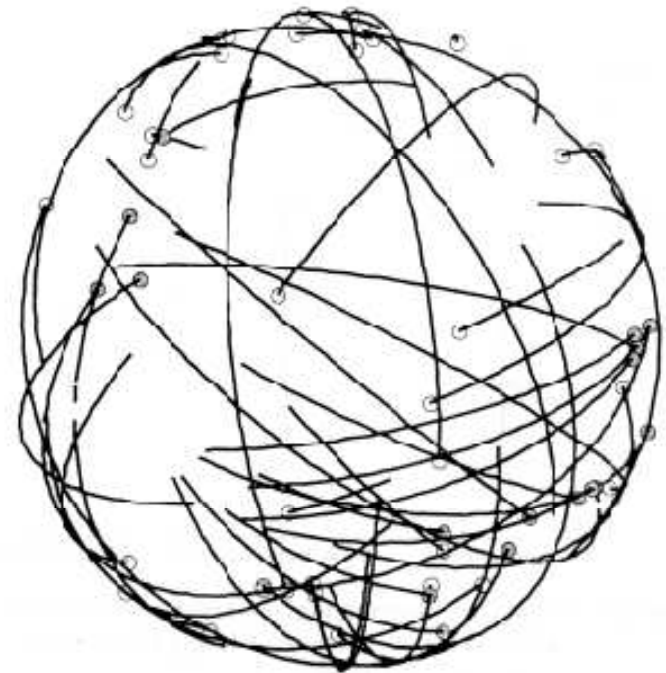

- Changes in preferred directions over time



Virtual Simulation

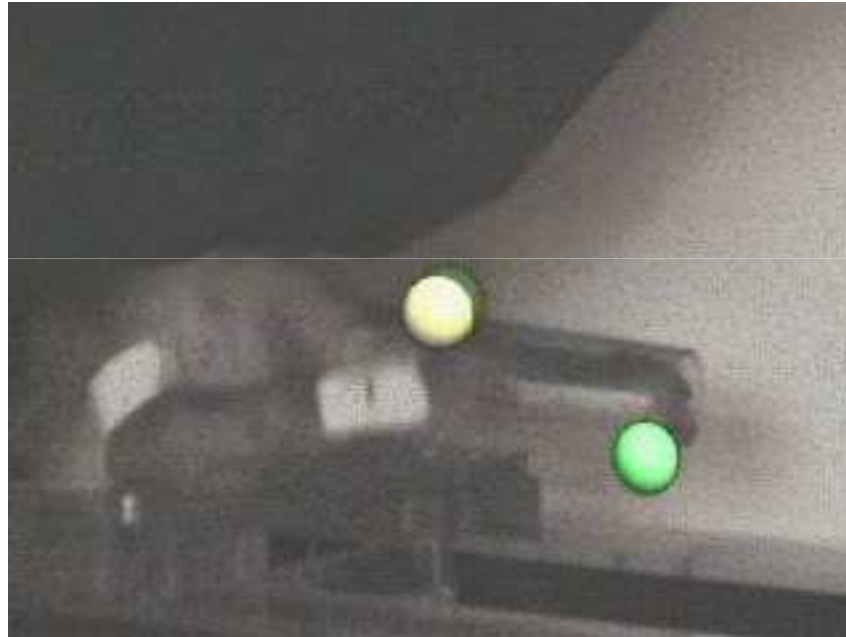


Prosthetic Testing



Video Source: [8]

Finger Licking Good






Conclusions

■ Reading

- Pros: sensory feedback, natural
- Cons: electrodes degrade, invasive, relies on functional nerves

■ Pittsburgh

- Pros: directly from motor cortex
- Cons: electrodes degrade, extremely invasive, only visual feedback



Next Steps

- Sensory feedback directly to sensory cortex



References

- [1] Gasson M, Hutt B, Goodhew I, Kyberd P, Warwick K. Invasive neural prosthesis for neural signal detection and nerve stimulation *International Journal of Adaptive Control and Signal Processing* v19 No. 5 p 365-375 2005
- [2] Warwick K, Gasson M, Hutt B, Goodhew I, Kyberd P, Andrews B, Teddy P, Shad A. The application of implant technology for cybernetic systems. *Archives of Neurology* 2003; 60(10):1369–1373.
- [3] Meel Velliste, Sagi Perel, M. Chance Spalding, Andrew S. Whitford & Andrew B. Schwartz, Cortical control of a prosthetic arm for self-feeding, *Nature*, 453, 1098-1101 (19 June 2008)
- [4] Helms Tillery SI, Taylor DM, Schwartz AB. Training in cortical control of neuroprosthetic devices improves signal extraction from small neuronal ensembles, *Rev Neurosci*. 2003;14(1-2):107-19.
- [5] van Hemmen L, Schwartx A. Population vector code: a geometric universal as actuator, *Biological Cybernetics*, vol 98, n6 2008
- [6] Brain pic <http://aids.hallym.ac.kr/d/kns/tutor/pns49.jpg>
- [7] <http://motorlab.neurobio.pitt.edu/multimedia.php>
- [8] Helms Tillery, S. I., Taylor, D. M. & Schwartz, A. B. The general utility of a neuroprosthetic device under direct cortical control. *Proc. 25th Annu. Int. Conf. IEEE EMBS* 3, 2043–2046 (2003).
- [9] Schwartz, A. B. Cortical neural prosthetics. *Annu. Rev. Neurosci.* 27, 487–507 (2004).
- [10] Kennedy P, Bakay R, Moore M, Adams K, Goldwaith J. Direct control of a computer from the human central nervous system. *IEEE Transactions on Rehabilitation Engineering* 2000; 8:198–202.
- [11] Kostov A, Polak M. Parallel Man-Machine Training in Development of EEG-Based Cursor Control *IEEE TRANSACTIONS ON REHABILITATION ENGINEERING*, VOL. 8, NO. 2, JUNE 2000
- [12] Gasson, M. Hutt, B. Goodhew, I. Kyberd, P. Warwick, K. Bi-directional human machine interface via direct neural connection *Robot and Human Interactive Communication*, 2002. *Proceedings. 11th IEEE International Workshop on*, 2002 p 265- 270
- [13] Adriano A, Nasuto S, Kyberd P, Sweeney-Reed C. Generative topographic mapping applied to clustering and visualization of motor unit action potentials, *Biosystems*, 2005, vol. 82, no3, pp. 273-284
- [14] F. Babiloni, F. Cincotti, L. Lazzarini, J. Millán, J. Mouriño, M. Varsta, J. Heikkonen, L. Bianchi, M. G. Marciani, Linear Classification of Low-Resolution EEG Patterns Produced by Imagined Hand Movements, *IEEE TRANSACTIONS ON REHABILITATION ENGINEERING*, VOL. 8, NO. 2, JUNE 2000
- [15] Birbaumer, N., Kubler, A., Ghanayim, N., Hinterberger, T., Perelmouter, J., Kaiser, J., Iversen, I., Kotchoubey, B., Neumann, N., & Flor, H. (2000). The thought translation device (ttd) for completely paralyzed patients. *Rehabilitation Engineering, IEEE Transactions on* , 8 (2), 190-193.
- [16] Robert E. Isaacs, D. J. Weber, and Aandrew B. Schwartz. Work Toward Real-Time Control of a Cortical Neural Prosthesis, *IEEE TRANSACTIONS ON REHABILITATION ENGINEERING*, VOL. 8, NO. 2, JUNE 2000